



International Conference on Industrial Engineering

Automated information-measurement system used to test the immunity of the medical equipment protective elements to the discharges of the defibrillator

Stetsenko I.A., Leuhin R.I., Shirokov K.M.*

Platov South-Russian State Polytechnic University (NPI), 132, St. Prosvescheniya, Rostov region, Novocherkassk, 346428, Russian Federation

Abstract

The article discusses the information-measurement system used for testing of protective elements medical equipment for their resistance to the discharge of a defibrillator, which is designed to test medical products, which may be exposed to high voltage defibrillator pulses, up to 5000 V while in operation. The Information-measurement system should provide a fully automated testing process in accordance with the international standard IEC 60601-1, as well as analyze the result and diagnose the parameters of elements the of a defibrillator block simulating the pulses.

© 2015 The Authors. Published by Elsevier Ltd. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Peer-review under responsibility of the organizing committee of the International Conference on Industrial Engineering (ICIE-2015)

Keywords: test medical devices for resistance to the pulse of defibrillator, the system of diagnostics of parameters of high voltage source.

1. Information-measuring system

To ensure the automation of the testing process of the developed information-measuring system that fully automates the testing process and allows [1][2][3] for self-diagnosis storage capacitor C3 of the high voltage [4] source [5][6][7]. The General scheme of application of the test voltage to the medical device [8] shown in figure 1.

* Corresponding author. Tel.: +7-863-525-5240; fax: +7-683-525-5240.
E-mail address: iimt-srstu@mail.ru

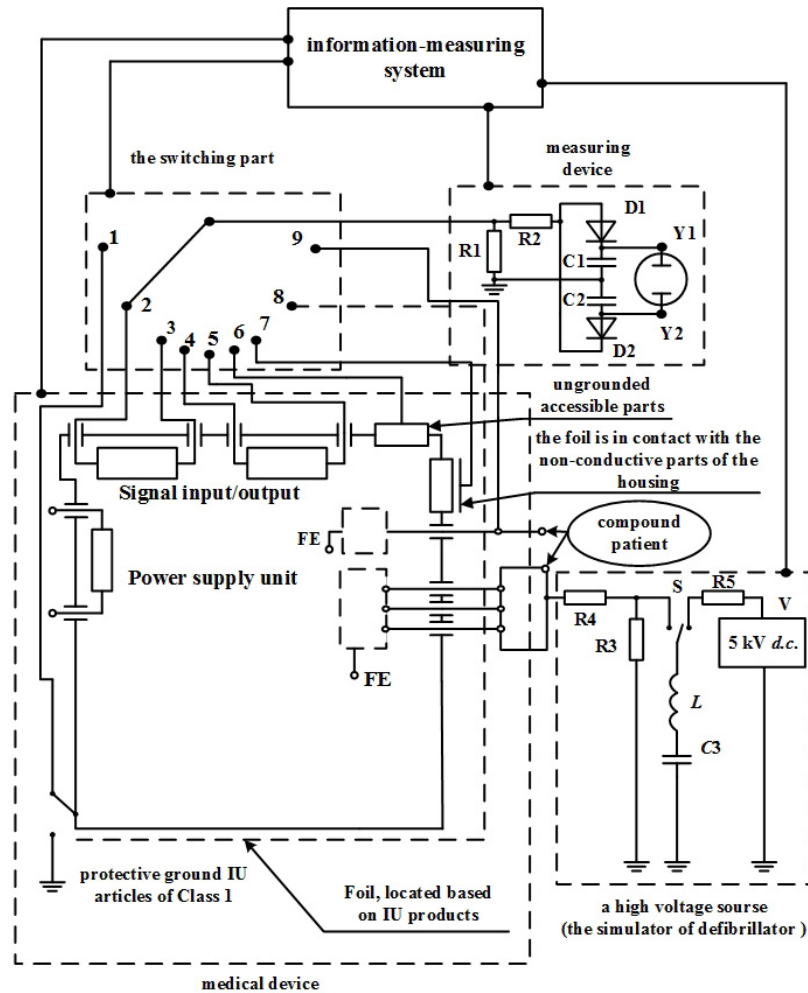


Fig. 1. The General scheme of application of test voltage to medical device

VT – test voltage, S – switch test voltage, R1, R2 - resistors with a tolerance of $\pm 2\%$ for voltage less than 2 kV, R3, R4 - resistors with a tolerance of $\pm 2\%$ for voltage less than 5 kV, R5 - limiting resistor, D1, D2 - miniature silicon small signal diodes (remaining components have a tolerance of $\pm 5\%$), 1 - the output of the switching control part, 2 – output of conclusion control the high voltage source, 3 - the sync output from the measuring.

2. Functions of IMS

The basic functions of the design information-measuring systems is the provision of a process of testing medical devices and self-diagnosis function of the parameters of the high voltage source such as the voltage on high voltage plates of capacitor C3 and its capacity[9][10][11]. In operation, the high voltage capacitor can change its settings and deviate from the values of the normalized standard[12][13].

The control voltage is produced by connecting the microprocessor control system to the terminals of the capacitor[14][15]. The program converts the analog signal into the voltage value on the capacitor plates. Resistors

R1, R2 form a voltage divider 5000/5 Volts. The scheme of connection of capacitor for the microprocessor shown in figure 2.

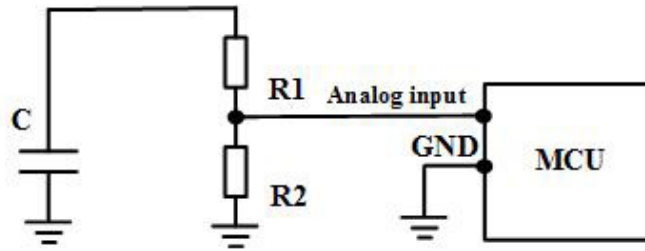


Fig. 2. The scheme of connection of the capacitor to the microprocessor
C - high voltage capacitor, R1, R2 – ladder, MCU – microprocessor.

A general algorithm for read voltage shown in the figure.3

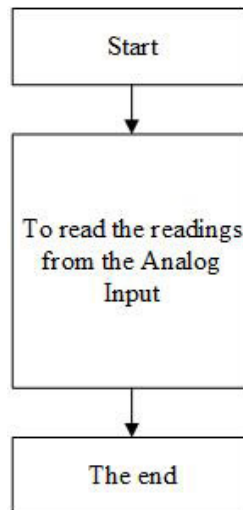


Fig.3. The general algorithm for read voltage.

The capacity control is performed by determining the time constant [16][17][18] of the capacitor charge, which is 63.2% of voltage a full charge, and is calculated by the formula (1)

$$\tau = R * C . \quad (1)$$

The scheme of connection of the capacitor to measure the capacitance shown in figure 4.

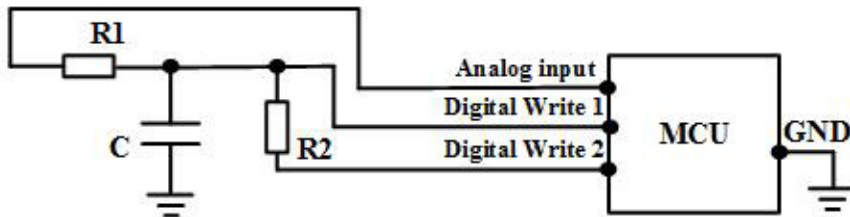


Fig. 4. The scheme of connection of the capacitor to measure the capacitance
 C - high voltage capacitor, R1- limiting resistor, R2 - resistor capacitor discharge, MCU – microprocessor.

A general algorithm for measuring the capacitance of the capacitor [19][20] shown in the figure.5

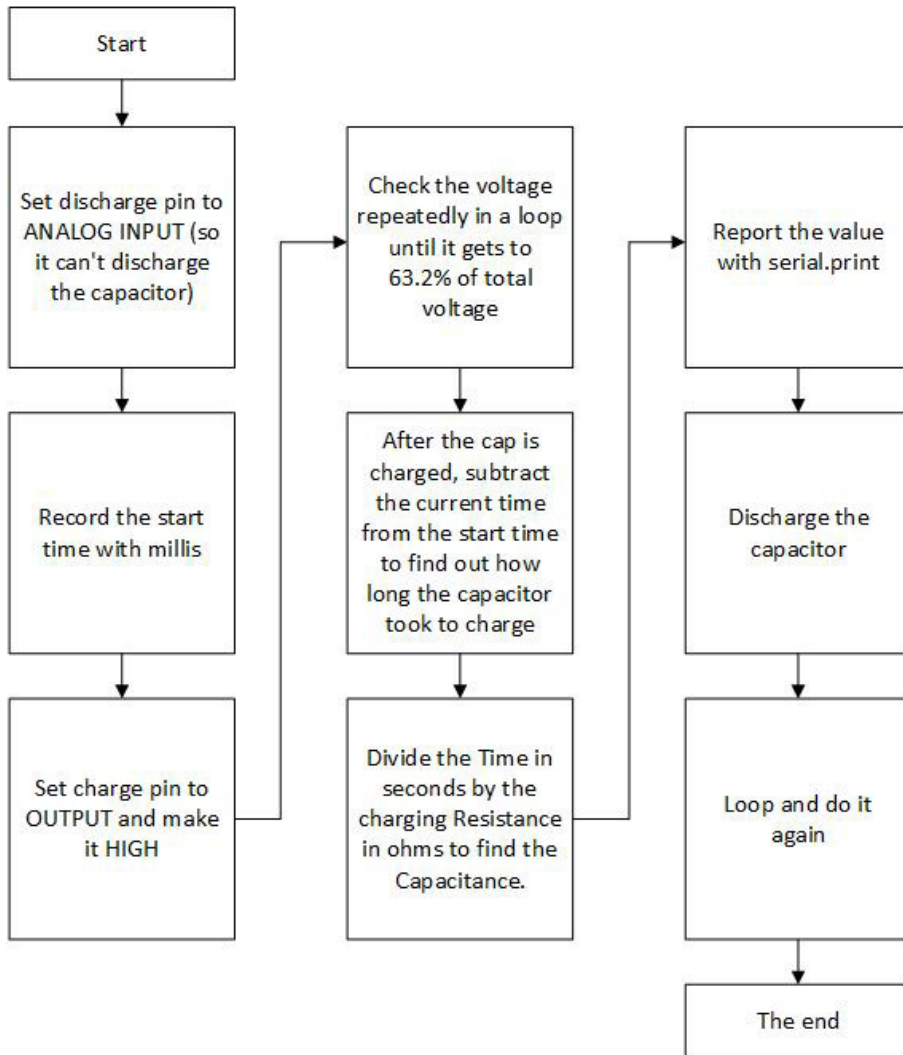


Fig.5. The algorithm for capacitance measurement.

3. Conclusion

Thus, the design of information-measuring system will ensure a process of testing medical equipment, but also possess the self-diagnosis function of the parameters of the high voltage source.

Acknowledgements

The project became the winner of the youth program Participant research scientific-innovation competition "P.R.S.I.C.". Project #4475GU1/214.

References

- [1] GOST R IEC 60601-1-2010 "Medical electrical equipment. Part 1: General requirements for safety on the major functional characteristics."
- [2] M.V. Lankin¹, N.I. Gorbatenko¹, I.A. Stetsenko¹, D.V. Shaikhutdinov¹, V.I. Dubrov¹, K.M. Shirokov, Automated test bench for security elements of medical equipment for resistance to defibrillator. SIBCON-2015, International Siberian Conference on Control and Communications, Omsk. (2015).
- [3] V.A. Vostrikov, B.B. Gorbunov, S.V. Selishchev, Construction of energy-optimal smooth monophasic defibrillation pulse waveforms using cardiomyocyte membrane model, *J Biomed Sci Eng.* 8(9) (2015) 625–631.
- [4] V.A. Vostrikov, B.B. Gorbunov, A.N. Gusev, I.V. Nesterenko, S.V. Selishchev, Determination of threshold energy level of monopolar defibrillation pulses using the Luo–Rudy cardiomyocyte model, *Biomedical Engineering.* (47)2 (2013) 61–64. DOI 10.1007/s10527-013-9335-8.
- [5] V.A. Vostrikov, B.B. Gorbunov, S.V. Selishchev, I.V. Venin Founder of biphasic waveform defibrillators, *J Biomed Sci Eng.* 8(5) (2015) 345–349.
- [6] V.A. Vostrikov, B.B. Gorbunov, I.V. Venin i ego vklad v razrabotku otechestvennykh defibrilljatorov, *Obshhaja reanimatologija.* 9(5) (2013) 68–73.
- [7] S. Zabodaev, I. Nesterenko, D. Telyshev, CPR artifact removal for providing continuous heart rate recovery procedure, *Proceedings of 1st Russian German Conference on Biomedical Engineering RGC, Germany.* (2013) 72.
- [8] V.A. Vostrikov, B.B. Gorbunov, A. Gusev, Comparison of the influence of the first phase of some biphasic defibrillation pulses on the cardiomyocyte model, *Proceedings of 1st Russian German Conference on Biomedical Engineering RGC 2013.* October, 23rd — 26th, 2013 Hannover, Germany. B. Cichkov, E. Fadeeva, L.A. Kahrs, T. Ortmaier, PZH Verlag, Germany. (2013) 14.
- [9] N.A. Bazaev, A.A. Danilov, A.Yu. Gerasimenko, B.B. Gorbunov, Yu.P. Masloboev, D.A. Potapov, D.V. Telyshev, S.A. Tereshchenko, S.V. Selishchev, Research and education complex for personnel training and basic and applied science research at the Biomedical Systems Department of the National Research University of Electronic Technology (MIET), *Biomedical Engineering.* (47)3 (2013) 111–115.
- [10] I.A. Stetsenko, Sh.V. Ahmedov, D.V. Shajhutdinov, R.I. Leuhin, Razrabotka algoritmov raboty stenda dlja ispytanij zashhitnykh jelementov medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora, *Teorija, metody i sredstva izmerenij, kontrolja i diagnostiki : materialy 15-oj Mezhdunar. nauch.-prakt. konf. Juzh.-Ros. gos. politehn. un-t (NPI) im. M.I. Platova, Novochoerkassk : JuRGPU.* (2014) 45–48.
- [11] D.V. Shajhutdinov, V.I. Dubrov, I.A. Stetsenko, Stend dlja ispytanij zashhitnykh jelementov medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora na baze tehnologij National instruments pech, *Nauka tret'ego tysjacheletija: sb. st. Mezhdunar. nauch.-prakt. konf., 5 sent, Ufa, Ajeterna.* (2014) 48–50.
- [12] I.A. Stetsenko, Stend dlja ispytanij zashhitnykh jelementov medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora na baze tehnologij National instruments, *Nauchno-tehnicheskaja konferencija i vystavka innovacionnykh proektov, vypolnennykh vuzami i nauchnymi organizacijami JuFO v ramkah uchastija v realizacii federal'nyh celevykh programm i vneprogrammyh meroprijatij, zakazchikom kotorykh javljaetsja Minobrnauki Rossii: sb. materialov konf., Juzh.-Ros. gos. politehn. un-t im. M.I. Platova, Novochoerkassk: Lik.* (2014) 112–114.
- [13] I.A. Stetsenko, Postroenie i analiz perehodnykh processov avarijnogo rezhima izmeritel'noj chasti stenda dlja ispytanija zashhitnykh chastej medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora v srede razrabotki NI MULTISIM, *Nauka: proshloe, nastojashhee, budushhee: sb. st. Mezhdunar. nauch.-prakt. konf., Nauch.-izdat. centr Ajeterna, Ufa.* 1 (2015) 65–68.
- [14] I.A. Stetsenko, Postroenie matematicheskoi modeli specializirovannogo istochnika pitaniya v sostave zarjada vysokovol'tnykh kondensatorov. *Sovremennij vzgljad na budushhee nauki: sb. st. Mezhdunar. nauch.-prakt. konf., Nauch.-izdat. centr "Ajeterna", Ufa.* 1 (2015) 44–49.
- [15] I.A. Stetsenko, Razrabotka specializirovannogo istochnika pitaniya i issledovanie ego raboty v sostave shemy zarjada vysokovol'tnykh kondensatorov, *Problemy i perspektivy tehniceskikh nauk: sb. st. Mezhdunar. nauch.-prakt. konf., NC Ajeterna, Ufa.* (2015) 39–43.
- [16] I.A. Stetsenko, Samodiagnostiruemyj istochnik pitaniya dlja stenda ispytanija medicinskoj apparatury, *Fundamental'nye problemy nauki: sb. st. Mezhdunar. nauch.-prakt. konf., Nauch.-izdat. centr "Ajeterna", Ufa.* 2 (2015) 57–58.
- [17] I.V. Venin, A.I. Red'ko, S.V. Serikov, V.Ja. Bersenev, Defibrilljatory: otechestvennaja istorija i priorityty, *Ekstrena medicina: vid nauki do praktiki.* 4(5) (2013) 125–131.
- [18] V.A. Vostrikov, B.B. Gorbunov, A.N. Gusev, S.V. Selishchev, Opredelenie porogovoj jenerгии monopoljarnykh defibrillirujushchih impul'sov s ispol'zovaniem modeli kardiomiocita Luo-Rudy, *Medicinskaja tehnika.* 2 (2013) 6–8.
- [19] S.S. Luksha, Portativnyj defibrilljator-monitor s funkciej kontrolja parametrov serdečno-sosudistoj sistemy, *Materialy XXIV Vserossijskoj nauchno-tehnicheskaja konferencija studentov, molodykh uchenykh i specialistov «BIOMEDSISTEMY – 2011».* (2012) 169–171

- [20] A.V. Il'ich, I.N. Bokarev, Resinhronizirujushhie ustrojstva s funkciej kardiostimuljatora /defibrilljatora, Klinicheskij opyt Dvadcatki. 4 (2012) 57–58.