



Available online at www.sciencedirect.com

ScienceDirect

Procedia Engineering 129 (2015) 239 – 244

**Procedia
Engineering**

www.elsevier.com/locate/procedia

International Conference on Industrial Engineering

Automated information-measurement system used to test the immunity of the medical equipment protective elements to the discharges of the defibrillator

Stetsenko I.A., Leuhin R.I., Shirokov K.M.*

Platov South-Russian State Polytechnic University (NPI), 132, St. Prosvescheniya, Rostov region, Novocherkassk, 346428, Russian Federation

Abstract

The article discusses the information-measurement system used for testing of protective elements medical equipment for their resistance to the discharge of a defibrillator, which is designed to test medical products, which may be exposed to high voltage defibrillator pulses, up to 5000 V while in operation. The Information-measurement system should provide a fully automated testing process in accordance with the international standard IEC 60601-1, as well as analyze the result and diagnose the parameters of elements the of a defibrillator block simulating the pulses.

© 2015 The Authors. Published by Elsevier Ltd. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Peer-review under responsibility of the organizing committee of the International Conference on Industrial Engineering (ICIE-2015)

Keywords: test medical devices for resistance to the pulse of defibrillator, the system of diagnostics of parameters of high voltage source.

1. Information-measuring system

To ensure the automation of the testing process of the developed information-measuring system that fully automates the testing process and allows [1][2][3] for self-diagnosis storage capacitor C3 of the high voltage [4] source [5][6][7]. The General scheme of application of the test voltage to the medical device [8] shown in figure 1.

* Corresponding author. Tel.: +7-863-525-5240; fax: +7-683-525-5240.

E-mail address: iimt-srstu@mail.ru

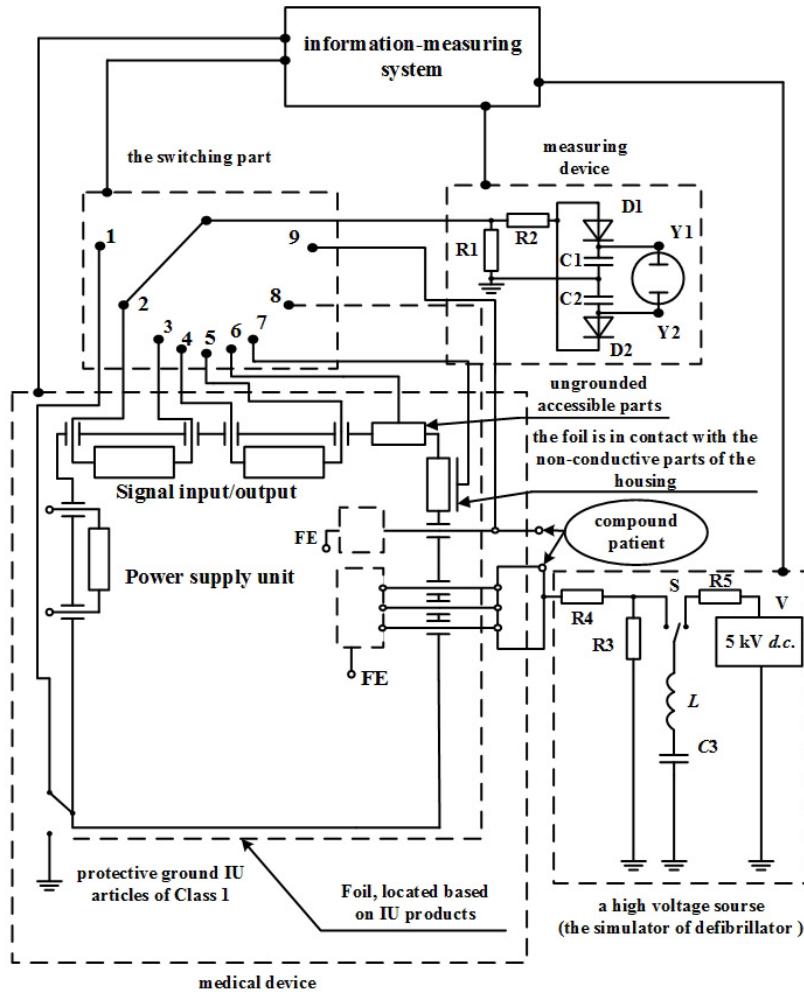


Fig. 1. The General scheme of application of test voltage to medical device

VT – test voltage, S – switch test voltage, R1, R2 - resistors with a tolerance of $\pm 2\%$ for voltage less than 2 kV, R3, R4 - resistors with a tolerance of $\pm 2\%$ for voltage less than 5 kV, R5 - limiting resistor, D1, D2 - miniature silicon small signal diodes (remaining components have a tolerance of $\pm 5\%$), 1 - the output of the switching control part, 2 – output of conclusion control the high voltage source, 3 - the sync output from the measuring.

2. Functions of IMS

The basic functions of the design information-measuring systems is the provision of a process of testing medical devices and self-diagnosis function of the parameters of the high voltage source such as the voltage on high voltage plates of capacitor C3 and its capacity[9][10][11]. In operation, the high voltage capacitor can change its settings and deviate from the values of the normalized standard[12][13].

The control voltage is produced by connecting the microprocessor control system to the terminals of the capacitor[14][15]. The program converts the analog signal into the voltage value on the capacitor plates. Resistors

R1, R2 form a voltage divider 5000/5 Volts. The scheme of connection of capacitor for the microprocessor shown in figure 2.

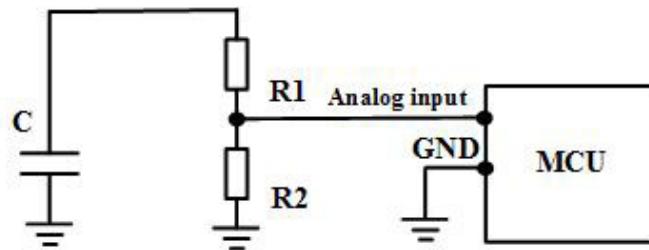


Fig. 2. The scheme of connection of the capacitor to the microprocessor
C - high voltage capacitor, R1, R2 – ladder, MCU – microprocessor.

A general algorithm for read voltage shown in the figure.3

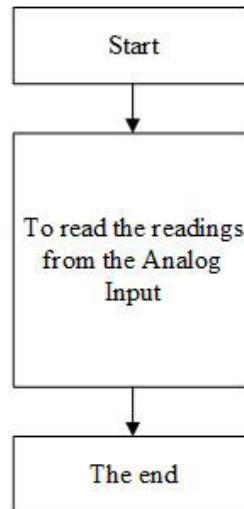


Fig.3. The general algorithm for read voltage.

The capacity control is performed by determining the time constant [16][17][18] of the capacitor charge, which is 63.2% of voltage a full charge, and is calculated by the formula (1)

$$\tau = R * C. \quad (1)$$

The scheme of connection of the capacitor to measure the capacitance shown in figure 4.

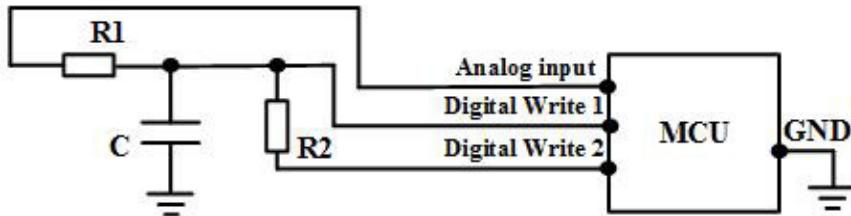


Fig. 4. The scheme of connection of the capacitor to measure the capacitance
C - high voltage capacitor, R1 - limiting resistor, R2 - resistor capacitor discharge, MCU – microprocessor.

A general algorithm for measuring the capacitance of the capacitor [19][20] shown in the figure.5

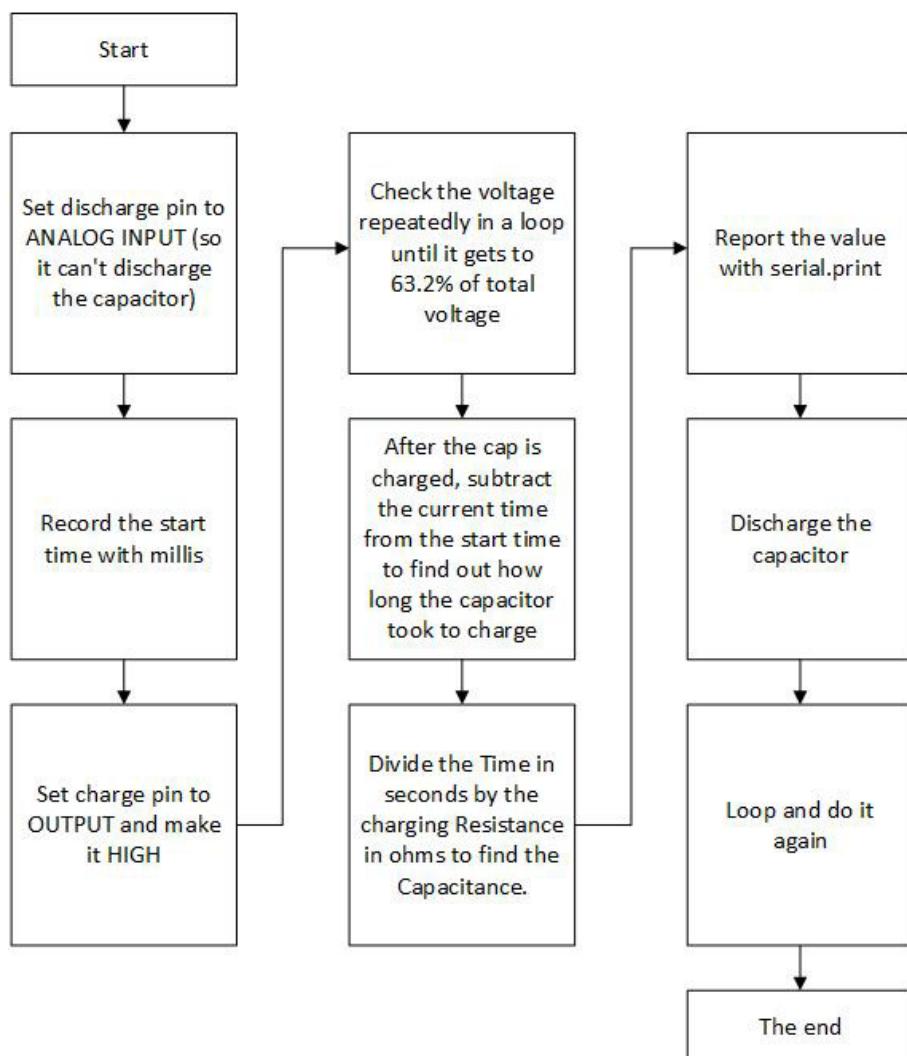


Fig.5. The algorithm for capacitance measurement.

3. Conclusion

Thus, the design of information-measuring system will ensure a process of testing medical equipment, but also possess the self-diagnosis function of the parameters of the high voltage source.

Acknowledgements

The project became the winner of the youth program Participant research scientific-innovation competition "P.R.S.I.C.". Project #4475GU1/214.

References

- [1] GOST R IEC 60601-1-2010 "Medical electrical equipment. Part 1: General requirements for safety on the major functional characteristics."
- [2] M.V. Lankin1, N.I. Gorbatenko1, I.A. Stetsenko1, D.V. Shaikhutdinov1, V.I. Dubrov1, K.M. Shirokov, Automated test bench for security elements of medi-cal equipment for resistance to defibrillator. SIBCON-2015, International Siberian Conference on Control and Communications, Omsk. (2015).
- [3] V.A. Vostrikov, B.B. Gorbunov, S.V. Selishchev, Construction of energy-optimal smooth monophasic defibrillation pulse waveforms using cardiomyocyte membrane model, J Biomed Sci Eng. 8(9) (2015) 625–631.
- [4] V.A. Vostrikov, B.B. Gorbunov, A.N. Gusev, I.V. Nesterenko, S.V. Selishchev, Determination of threshold energy level of monopolar defibrillation pulses using the Luo-Rudy cardiomyocyte model, Biomedical Engineering. (47)2 (2013) 61–64. DOI 10.1007/s10527-013-9335-8.
- [5] V.A. Vostrikov, B.B. Gorbunov, S.V. Selishchev, I.V. Venin Founder of biphasic waveform defibrillators, J Biomed Sci Eng. 8(5) (2015) 345–349.
- [6] V.A. Vostrikov, B.B. Gorbunov, I.V. Venin i ego vklad v razrabotku otechestvennyh defibrilljatorov, Obshhaja reanimatologija. 9(5) (2013) 68–73.
- [7] S. Zabodaev, I. Nesterenko, D. Telyshev, CPR artifact removal for providing continuous heart rate recovery procedure, Proceedings of 1st Russian German Conference on Biomedical Engineering RGC, Germany. (2013) 72.
- [8] V.A. Vostrikov, B.B. Gorbunov, A. Gusev, Comparison of the influence of the first phase of some biphasic defibrillation pulses on the cardiomyocyte model, Proceedings of 1st Russian German Conference on Biomedical Engineering RGC 2013. October, 23rd — 26th, 2013 Hannover, Germany. B. Cichkov, E. Fadeeva, L.A. Kahrs, T. Ortmaier, PZH Verlag, Germany. (2013) 14.
- [9] N.A. Bazaev, A.A. Danilov, A.Yu. Gerasimenko, B.B. Gorbunov, Yu.P. Masloboev, D.A. Potapov, D.V. Telyshev, S.A. Tereshchenko, S.V. Selishchev, Research and education complex for personnel training and basic and applied science research at the Biomedical Systems Department of the National Research University of Electronic Technology (MIET), Biomedical Engineering. (47)3 (2013) 111–115.
- [10] I.A. Stecenko, Sh.V. Ahmedov, D.V. Shajhutdinov, R.I. Leuhin, Razrabotka algoritmov raboty stenda dlja ispytanij zashhitnyh jelementov medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora, Teoriya, metody i sredstva izmerenij, kontrolja i diagnostiki : materialy 15-oj Mezhdunar. nauch.-prakt. konf., Juzh.-Ros. gos. politehn. un-t (NPI) im. M.I. Platova, Novocherkassk : JuRGPU. (2014) 45–48.
- [11] D.V. Shajhutdinov, V.I. Dubrov, I.A. Stetsenko, Stend dlja ispytanij zashhitnyh jelementov medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora na baze tehnologij National instruments pech, Nauka tre'tego tysjacheletija: sb. st. Mezhdunar. nauch.-prakt. konf., 5 sent, Ufa, Ajeterna. (2014) 48–50.
- [12] I.A. Stetsenko, Stend dlja ispytanij zashhitnyh jelementov medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora na baze tehnologij National instruments, Nauchno-tehnicheskaja konferencija i vystavka innovacionnyh proektor, vypolnenyyh vuzami i nauchnymi organizacijami JuFO v ramkah uchastija v realizacii federal'nyh celevyh programm i vneprogrammnyh meroprijatij, zakazchikom kotoryh javljaetsja Minobrnauki Rossii: sb. materialov konf., Juzh.-Ros. gos. politehn. un-t im. M.I. Platova, Novocherkassk: Lik. (2014) 112–114.
- [13] I.A. Stetsenko, Postroenie i analiz perehodnyh processov avarijnogo rezhma izmeritel'noj chasti stenda dlja ispytaniya zashhitnyh chastej medicinskoj apparatury na ustojchivost' k razrjadam defibriljatora v srede razrabotki NI MULTISIM, Nauka: proshloe, nastojashhee, budushhee: sb. st. Mezhdunar. nauch.-prakt. konf., Nauch.-izdat. centr Ajeterna, Ufa. 1 (2015) 65–68.
- [14] I.A. Stetsenko, Postroenie matematicheskoy modeli specializirovannogo istochnika pitanija v sostave zarjada vysokovol'tnyh kondensatorov. Sovremennyj vzgljad na budushhee nauki: sb. st. Mezhdunar. nauch.-prakt. konf., Nauch.-izdat. centr "Ajeterna", Ufa. 1 (2015) 44–49.
- [15] I.A. Stetsenko, Razrabotka specializirovannogo istochnika pitanija i issledovanie ego raboty v sostave shemy zarjada vysokovol'tnyh kondensatorov, Problemy i perspektivy tehnicheskikh nauk: sb. st. Mezhdunar. nauch.-prakt. konf., NC Ajeterna, Ufa. (2015) 39–43.
- [16] I.A. Stetsenko, Samodiagnostireuyj istochnik pitanija dlja stenda ispytaniya medicinskoj apparatury, Fundamental'nye problemy nauki: sb. st. Mezhdunar. nauch.-prkt. konf., Nauch.-izdat. centr "Ajeterna", Ufa. 2 (2015) 57–58.
- [17] I.V. Venin, A.I. Red'ko, S.V. Serikov, V.Ja. Bersenev, Defibrillatory: otechestvennaja istorija i prioritety, Ekstrena medicina: vid nauki do praktiki. 4(5) (2013) 125–131.
- [18] V.A. Vostrikov, B.B. Gorbunov, A.N. Gusev, S.V. Selishchev, Opredelenie porogovoj jenergii monopoljarnyh defibrillirujushhih impul'sov s ispol'zovaniem modeli kardiomiocita Luo-Rudy, Medicinskaja tekhnika. 2 (2013) 6–8.
- [19] S.S. Luksha, Portativnyj defibrillator-monitor s funkcijs kontrolja parametrov serdechno-sosudistoj sistemy, Materialy XXIV Vserossijskoy nauchno-tehnicheskaja konferencija studentov, molodyh uchenyh i specialistov «BIOMEDSISTEMY – 2011», (2012) 169–171

- [20] A.V. Il'ich, I.N. Bokarev, Resinhronizirujushhie ustrojstva s funkciej kardiostimulyatora /defibrilljatora, Klinicheskij opyt Dvadcatki. 4 (2012) 57–58.